



Original article

Dispersive liquid-liquid microextraction, an effective tool for the determination of synthetic cannabinoids in oral fluid by liquid chromatography–tandem mass spectrometry



Pierpaolo Tomai^a, Alessandra Gentili^{a,*}, Roberta Curini^a, Rossella Gottardo^b, Franco Tagliaro^b, Salvatore Fanali^c

^a Department of Chemistry, Sapienza University, P.le Aldo Moro 5, 00185, Rome, Italy

^b Department of Diagnostics and Public Health, University of Verona, Verona, Italy and Institute of Translational Medicine and Biotechnology, Sechenov First Moscow State Medical University, Moscow, Russia

^c Teaching Committee of Ph.D. School in Natural Science and Engineering University of Verona, Verona, Italy

ARTICLE INFO

Article history:

Received 9 April 2020

Received in revised form

12 November 2020

Accepted 16 November 2020

Available online 19 November 2020

Keywords:

Microextraction techniques

Dispersive liquid-liquid microextraction

Illicit drugs

Synthetic cannabinoids

Silica C-based column

ABSTRACT

In the present work, dispersive liquid-liquid microextraction (DLLME) was used to extract six synthetic cannabinoids (JWH-018, JWH-019, JWH-073, JWH-200, or WIN 55,225, JWH-250, and AM-694) from oral fluids. A rapid baseline separation of the analytes was achieved on a bidentate octadecyl silica hydride phase (Cogent Bidentate C₁₈; 4.6 mm × 250 mm, 4 μm) maintained at 37 °C, by eluting in isocratic conditions (water:acetonitrile (25:75, V/V)). Detection was performed using positive electrospray ionization–tandem mass spectrometry. The parameters affecting DLLME (pH and ionic strength of the aqueous phase, type and volume of the extractant and dispersive solvent, vortex and centrifugation time) were optimized for maximizing yields. In particular, using 0.5 mL of oral fluid, acetonitrile (1 mL), was identified as the best option, both as a solvent to precipitate proteins and as a dispersing solvent in the DLLME procedure. To select an extraction solvent, a low transition temperature mixture (LTTM; composed of sesamol and chlorine chloride with a molar ratio of 1:3) and dichloromethane were compared; the latter (100 μL) was proved to be a better extractant, with recoveries ranging from 73% to 101% by vortexing for 2 min. The method was validated according to the guidelines of Food and Drug Administration bioanalytical methods: intra-day and inter-day precisions ranged between 4% and 18% depending on the spike level and analyte; limits of detection spanned from 2 to 18 ng/mL; matrix-matched calibration curves were characterized by determination coefficients greater than 0.9914. Finally, the extraction procedure was compared with previous methods and with innovative techniques, presenting superior reliability, rapidity, simplicity, inexpensiveness, and efficiency.

© 2020 Xi'an Jiaotong University. Production and hosting by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

1. Introduction

Synthetic cannabinoids (SCs) include a considerably large family of compounds, but only a few of them are structurally related to the primary psychoactive component of cannabis, Δ⁹-tetrahydrocannabinol (Δ⁹-THC) [1]. Most SCs are 3-indole derivatives, usually referred to by trade names related to their devisers, e.g., JWH-XXX (John W Huffmann) [2], CP-XX, XXX (Charles Pfizer), HU-XXX (Hebrew University), and AM-XXXX (Alexandros Makriyannis).

Within a trade name group, several chemical subgroups are included, such as benzoyl, naphthol, phenylacetyl, alkyl, piperazinyl, carboxylate, carboxamide, thiazolyl, and naphthylmethyl derivatives [1,3]. In this context, the JWH series represents one of the main SC subgroups detected in herbal products, with brand names such as “Spice”, “K2”, “herbal incense”, “Cloud 9”, and “Mojo” [4]. These apparently innocuous articles are sold on the Internet or in convenience stores disguised as products to perfume the environment or for other unoffending purposes. The direct consequence of this easy availability is the widespread abuse of such drugs, especially among younger individuals in whom an increasing number of intoxication cases have been recorded. To curb the circulation of these products, control institutions need

Peer review under responsibility of Xi'an Jiaotong University.

* Corresponding author.

E-mail address: alessandra.gentili@uniroma1.it (A. Gentili).

quick, simple, and reliable analytical methods to perform analyses of a large number of biological and seized specimens containing the target and/or unidentified SCs. To date, most analytical methodologies developed rely on gas chromatography and liquid chromatography coupled with mass spectrometry (GC-MS and LC-MS). In clinical and forensic toxicology, in addition to serum/blood [5–8] and herbal blends [9–12], methods of special interest are also being developed to screen and/or confirm the occurrence of SCs in “non-invasive” biological matrices such as urine [13–16] and saliva [17–22], with the latter considered as one of the most accessible biological fluids. In particular, oral fluid analysis has proved to be a practical solution for the detection of SCs, especially during roadside or workplace drug testing. Moreover, saliva collection is a simple procedure that does not require the presence of medical staff. To date, methods analyzing SCs in the oral fluid have employed conventional extraction procedures based on liquid-liquid extraction (LLE) or solid-phase extraction (SPE). Although valid, these approaches fail to adequately meet the high throughput requirements implemented owing to the need to monitor a significant number of samples. Dispersive liquid-liquid micro-extraction (DLLME) is a valid technique for the extraction of several classes of compounds from aqueous environmental samples [23,24]; rapidity is one of its distinct merits. Nevertheless, its application in the treatment of biological fluids warrants the proper selection of a dispersing solvent, which should allow both dispersion of the extractant in the aqueous sample and precipitation of peptides and proteins. This aspect is nearly always neglected [25–27], and if not precisely addressed, it can be responsible for: i) an imperfect separation between the aqueous and organic phases after the DLLME centrifugation step, ii) difficulty in recovering the settled phase, and iii) stress on the chromatographic system.

In the present work, for the first time, a DLLME procedure was developed to extract SCs from oral fluids. The new extraction procedure was carefully evaluated and organized to overcome the above-mentioned analytical problems. Accordingly, special attention was paid to the two-fold role that the dispersing solvent should satisfy when DLLME is applied to biological fluids and, particularly, to saliva. High-performance liquid chromatography–tandem mass spectrometry (HPLC-MS) was used for analyte quantitative determination. Once optimized, the DLLME method was compared with conventional SPE, as well as innovative solutions (DLLME based on the use of a deep eutectic solvent as extraction solvent; rotating disc-SPE using buckypaper), to achieve the best results. Finally, this work incorporated innovative experiments on i) the chromatographic behavior of these analytes on a bidentate C_{18} silica hydride phase in comparison with a conventional C_{18} , and ii) the optimization of an isocratic separation, which is another important time-saving strategy in clinical or forensic routine investigations.

2. Materials and methods

2.1. Chemicals, materials, and solutions

The analytical standards of JWH-018, JWH-019, JWH-073, JWH-200, JWH-250, and AM-694 were obtained from LGC Standards (Sesto San Giovanni, Milan, Italy). The exact masses and log P of the analytes are shown in Fig. 1. Choline chloride and sesamol, with purity grade greater than 98%, methanol, ethanol, acetonitrile, ethyl acetate, tetrahydrofuran (THF), chloroform (RS-PLUS grade), and formic acid (50%, V/V) were purchased from Sigma-Aldrich. Commercial buckypaper (BP) was purchased from Nanolab, Inc. (Nanolab, Waltham, USA). Oasis HLB cartridges (500 mg, 6 mL) were purchased from Waters Corporation (Milford, MA, USA). Ultrapure water was obtained using a Milli-Q water generator (Millipore, Bedford, MA, USA). Individual stock solutions were prepared

in methanol at a concentration of 1 mg/mL. Working standard solutions were prepared by diluting the stock solutions with methanol at proper concentrations according to the various stages of the experimental work. All solutions were stored at $-20\text{ }^{\circ}\text{C}$.

2.2. Liquid chromatography–tandem mass spectrometry

The samples were analyzed with a PerkinElmer series 200 HPLC system equipped with an autosampler (PerkinElmer, Norwalk, CT). Chromatographic separation was performed on a Cogent Bidentate C_{18} (4.6 mm \times 250 mm, 4 μm) column (MTC, Eatontown, NJ, USA) maintained at $37\text{ }^{\circ}\text{C}$. The analysis time of a single run was 15 min using isocratic conditions: water:acetonitrile (25:75, V/V) at a flow rate of 1 mL/min. The mobile phase was split employing a post-column T-valve, leading to 200 $\mu\text{L}/\text{min}$ into the electrospray ionization (ESI) source of the mass spectrometer. After each injection, the autosampler needle was washed with acetonitrile.

The analytes were detected with a PE-Sciex API-3000[®] (PerkinElmer Sciex Toronto, Canada) triple quadrupole mass spectrometer. The ESI source was operated in positive ionization with a capillary voltage of +4500 V. High purity nitrogen was used both as curtain gas and collision gas, while air was employed as the nebulizer gas and drying gas. The latter was heated by adjusting the source heater temperature to $350\text{ }^{\circ}\text{C}$. The full width at half maximum (FWHM) was set at $m/z\ 0.7 \pm 0.1$ in each mass-resolving quadrupole to operate with a unit resolution. The multiple reaction monitoring (MRM) mode was used for analyte quantification. Two MRM transitions were selected per analyte, for a total of 12 ion currents monitored with a pause time of 5 ms. All LC–MS parameters useful for identification and quantification are listed in Table 1. The LC–MS data were processed using Analyst[®] 1.5 Software (AB Sciex).

2.3. Sample collection

For the optimization and validation of the DLLME method, oral fluid was collected from healthy volunteers ($n = 5$) after obtaining consent. Each sample (approximately 1 mL) was directly collected into a 15-mL polypropylene tube, 30 min after a meal or after tooth brushing to obtain residue-free samples. The saliva from different donors was pooled (20 mL) and used for method validation. The samples were maintained at $-20\text{ }^{\circ}\text{C}$ until use.

2.4. Preparation of chlorine chloride(sesamol)₃

For a low transition temperature mixture (LTTM) preparation, both choline chloride and sesamol were dried individually in an oven at $50\text{ }^{\circ}\text{C}$ for 24 h. The solid mixture of the two components was prepared by weighing 1.000 g of choline chloride and 1.979 g of sesamol to achieve a molar ratio of 1:3. Next, the solid mixture was heated at $50\text{ }^{\circ}\text{C}$ to favor the quick formation of an amber viscous liquid (4 mL). The LTTM was cooled and later stored at room temperature until use. For extraction, the LTTM was slightly heated to reduce its viscosity and favor its sampling using a microsyringe.

2.5. Sample preparation

The extraction procedure for SCs from oral fluid involved two steps: i) protein precipitation and ii) DLLME procedure.

2.5.1. Protein precipitation

An aliquot of 0.5 mL of oral fluid was placed into a 15 mL centrifuge tube, and 1 mL of ice-cold acetonitrile was added. The mixture was sonicated for 5 min to promote protein precipitation and centrifuged at 12,500 g for 5 min. The supernatant was

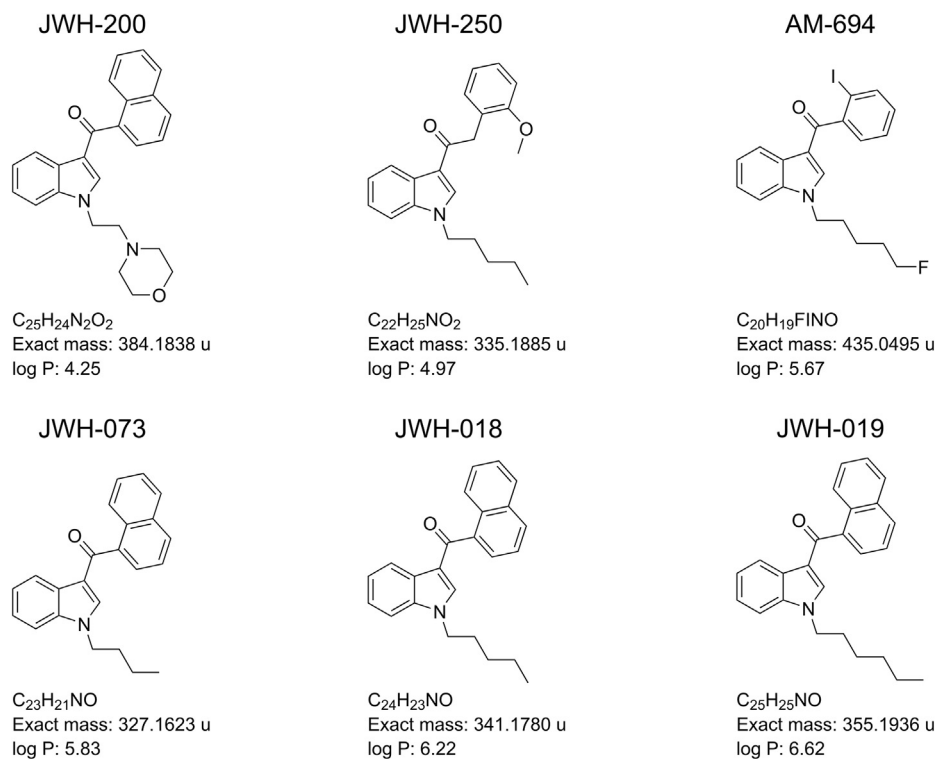


Fig. 1. Structures, exact masses and log P of the synthetic cannabinoids selected for this study.

transferred to a 15 mL centrifuge tube for the subsequent DLLME step.

2.5.2. DLLME procedure

The supernatant obtained in the previous step (about 1.5 mL) was diluted with 4.5 mL of water; acetonitrile (used for protein precipitation) acted as a dispersing solvent. Thus, 100 μ L of chloroform (extraction solvent) was directly injected into the supernatant. The mixture was vigorously vortexed for 2 min to favor the formation of a cloudy solution. After centrifugation at 12,500 g for 5 min, the settled phase was isolated using a microsyringe, transferred into another tube, and evaporated to dryness under nitrogen flow in a water bath at 40 °C. The residue was reconstituted with 50 μ L of water:methanol (25:75, V/V) and injected into the HPLC-MS system (5 μ L).

2.6. Method validation

The DLLME-HPLC-MS method for the analysis of SCs in oral fluids was validated by assessing recovery, precision, linearity, limit of detection (LOD), and lower limit of quantitation (LLOQ). The most intense MRM transition (MRM₁) was used for quantitative purposes and to calculate LOD and LLOQ, whereas the second most intense one (MRM₂) was chosen for confirmation purposes.

When required, blank samples were spiked pre-extraction with the analytes and vortexed for 5 min to favor their mixing with the matrix. Recoveries and precisions (intra-day and inter-day) were evaluated at the LLOQ and 10 times the LLOQ, analyzing five replicates for each spike level on the same day. Inter-day precision was evaluated by analyzing 10 replicates over a two-week period.

Matrix-matched calibration curves were built by spiking six blank aliquots with increasing concentrations of the analytes (0.00, 0.03, 1, 10, 20, 35, and 50 ng/mL) pre-extraction. The curves were

constructed by linear regression, plotting the peak area against the spike level.

LOD and LLOQ were experimentally estimated as the minimum concentration of an analyte in oral fluid capable of providing a signal-to-noise ratio of 3 and 5, respectively.

3. Results and discussion

3.1. Optimization of the chromatographic conditions

Based on the chemical structure of the evaluated SCs and their physico-chemical properties (log P) (see Fig. 1), C₁₈ silica stationary

Table 1

LC-MS parameters used for the six synthetic cannabinoids (SCs) identification in oral fluid samples. Retention time and ion ratio were calculated as mean of three replicates.

Analyte	Retention time (min)	MRM transition ^a (m/z)	Ion ratio ^b (%)
AM-694	4.77 ± 0.02	436.1/231.0	31
		436.1/203.1	
JWH-250	6.22 ± 0.02	336.2/121.2	10
		336.2/200.2	
JWH-073	6.78 ± 0.03	328.2/155.2	50
		328.2/126.9	
JWH-018	7.89 ± 0.02	342.2/155.2	54
		343.0/126.9	
JWH-019	9.42 ± 0.03	356.2/155.2	56
		356.2/127.2	
JWH-200	12.55 ± 0.09	385.2/155.2	49
		385.2/114.2	

^a The first line and the second line report the most intense MRM transition (MRM₁) and the second most intense one (MRM₂), respectively.

^b The ion ratio (relative abundance) between the two MRM transitions is calculated as MRM₂ intensity/MRM₁ intensity; the results are reported as arithmetic average of three replicates.

phases were considered for separation. Accordingly, two columns were tested: a C₁₈ Cogent bidentate silica C (4.6 mm × 250 mm, 4 μm) and an XTerra MS C₁₈ (4.6 mm × 250 mm, 5 μm). Different mobile phases, containing mixtures of water:methanol or water:acetonitrile, ranging between 60% and 100% (V/V) of organic solvent, as well as different column temperatures (25, 30, 37, 40, 45, 50, 55 °C), were assessed for the HPLC separation of compounds under investigation.

For chromatographic applications, the C₁₈ Cogent bidentate silica C is known to be advantageous because it has a limited number of non-polar silicon hydride (Si–H) groups and is effective for the separation of both hydrophobic and polar analytes [28]. The best results, in terms of chromatographic efficiency and baseline resolution, were obtained by elution with acetonitrile:water (75:25, V/V) at 37 °C; these conditions allowed the complete separation of AM-694, JWH-250, JWH-073, JWH-018, JWH-019, and JWH-200 in approximately 14 min. Conversely, on the XTerra MS C₁₈, a conventional silica phase end-capped column, analyte separation was accomplished within 8 min, but two analytes (JWH-200/AM-694 and JWH-250/JWH-073) were not separated at the baseline. Figs. 2A and B present the separation of SCs on the bidentate and end-capped C₁₈ stationary phases, respectively.

As demonstrated, the selectivities of the two columns differed, especially for JWH-200, the analyte that possesses the lowest log P value. On the end-capped column, the interaction took place according to the compound hydrophobicity (JWH-200 was the first to elute), while contrasting behavior was observed on the bidentate column, from which JWH-200 was the last SC to elute. The different selectivity achieved for this compound with the bidentate stationary phase can be explained by considering the basicity of the morpholine nitrogen (the other SCs are neutral compounds; see Fig. 1) and other factors such as steric hindrance and/or bonding of octadecyl to silica. Furthermore, it is interesting to highlight that the chromatographic retention of JWH-200 on the Cogent column was particularly influenced by temperature. In general, it is well known that an increase in column temperature can influence analyte retention, mainly due to changes in the mobile phase viscosity [29]. As expected, in this study, a temperature increase in the range of 25–55 °C decreased retention times of all evaluated compounds on both C₁₈ columns. However, the effect was more pronounced for JWH-200 on the bidentate column: it was the most retained analyte for temperatures less than 45 °C; however, above this value, it showed retention similar to that of JWH-019 (45 °C) and JWH-018 (55 °C), resulting in the loss of the baseline separation.

3.2. Optimization of the extraction conditions

Oral fluid is a biological solution containing water (more than 97%), cells, enzymes, glycoproteins such as mucins, minerals, and other organic compounds (e.g., urea, uric acid, cholesterol, vitamins, and phospholipids) [30]. In addition to this complexity, oral fluid poses additional pre-analytical challenges owing to its viscosity and surface tension. Moreover, the DLLME procedures that have been applied to this matrix [25–27] have failed to employ a preliminary deproteinization step, hindering the achievement of good phase separation, as well as the recovery of the settled phase. As typically observed in DLLME, these procedures are based on the direct injection of a balanced solution composed of dispersing solvent and extraction solvent into the aqueous biological sample, resulting in the unavoidable formation of a protein precipitate [25,26].

Hence, the first experiments performed in this study were aimed at optimizing protein precipitation by testing different analytical solutions. In all tests, 0.5 mL aliquots of a pool of oral fluid were used and spiked with the target analytes at 2 ng/mL.

Chloroform (100 μL) and other organic solvents (acetonitrile, THF, ethanol, or ethyl acetate) were used as extraction and dispersing solvents and vortexed for 5 min to form the cloudy solution.

Initially, the oral fluid was directly centrifuged at 12,500 g for 5 min. This approach allowed only partial protein precipitation; furthermore, when DLLME was performed, additional protein precipitate was formed following the contact of the oral fluid with the balanced solution of the dispersing (1 mL of acetonitrile) and extracting solvents.

The second approach evaluated the addition of an organic solvent (acetonitrile, THF, acetonitrile, ethanol, or ethyl acetate) to be used as the dispersing solvent in the DLLME experiments. The first attempts involved diluting the oral fluid (0.5 mL) with Milli-Q water to obtain a final volume of 5 mL. Subsequently, a solution of dispersing solvent (0.5 mL or 1 mL) and chloroform (100 μL) was prepared and quickly injected into the aqueous sample. After vortexing and centrifugation, in all cases, an abundant precipitate prevented the recovery of the settled chlorinated phase at the bottom of the centrifuge tube. To avoid this inconvenience, protein precipitation was achieved by treating the oral fluid directly with the dispersing solvent. Except for ethyl acetate and partly THF (effective using only 1 mL), all other solvents (acetonitrile and ethanol) were able to precipitate proteins efficiently using either 0.5 mL or 1 mL. After centrifugation at 12,500 g for 5 min, the supernatant (1 mL or 1.5 mL, depending on the volume used) was diluted with Milli-Q water up to 5 mL. On injecting 100 μL of chloroform into the diluted sample, the best extraction yields were achieved using 1 mL of acetonitrile. To further improve recoveries, both pH (4 and 9) and ionic strength (NaCl concentrations of 50, 100, and 200 mg/mL) of the sample were varied; however, as expected, the results demonstrated that the effect of these parameters on obtained yields was not significant owing to the neutral nature of the SCs (pH) and the proper selection of the extraction solvent (no further advantages from the salting-out effect due to the increased ionic strength). Finally, comparative experiments (vortex and ultrasound tested for 1, 2, 5, and 10 min) showed that a finely dispersed solution was easily obtained after vortexing for 2 min.

During this phase of experimentation, a further attempt to increase the extraction efficiency was undertaken by testing an LTTM as the extraction solvent. Maintaining all conditions of the optimized procedure with chloroform, the effect of chlorine chloride (sesamol)₃ (100 μL) was assessed. Unfortunately, acetonitrile was unable to disperse the LTTM in the aqueous sample, and hence, a new optimization study identified THF (1 mL) as a more suitable solvent. In this case, the pH and ionic strength were not relevant, while the best dispersion conditions were obtained by applying 5 min of ultrasound.

Fig. 3 shows the comparison between the two developed DLLME methods. On employing LTTM as an extractant, recoveries ranged from 41% to 108%. Superior results were obtained with chloroform, which permitted recoveries greater than 85%.

3.3. Method validation

All figures of merit of the validated method are reported in Table 2.

Matrix-matched calibration curves were constructed by spiking five aliquots of oral fluid (each 0.5 mL) with increasing concentrations of the analytes (0.03, 1, 10, 20, 30, 40, and 50 ng/mL); an unspiked aliquot was used as a “zero concentration” sample. Extraction and analysis were performed according to the procedure described in the Experimental Section. The peak area and concentration were linearly related to determination coefficients (R²) greater than 0.9914, as shown in Fig. S1.

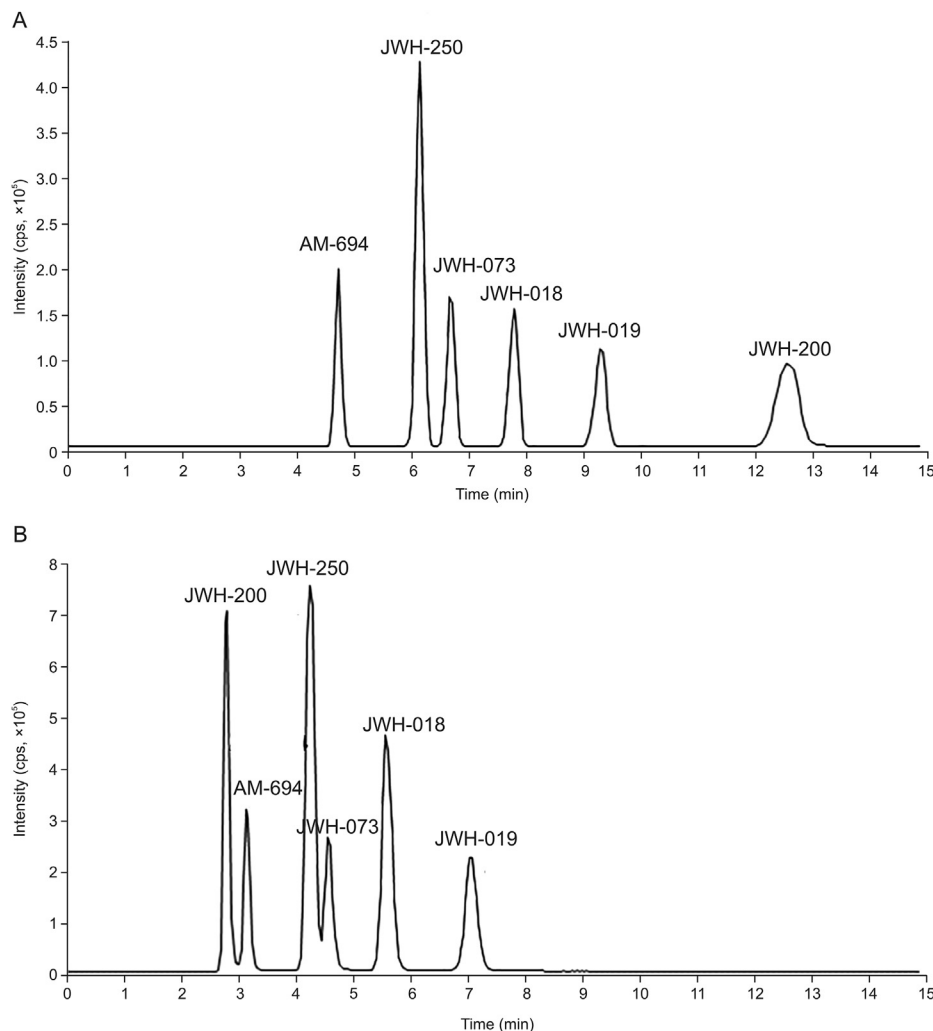


Fig. 2. Chromatographic separation of the selected cannabinoids on (A) a bidentate C₁₈ silica hydride phase and on (B) an end-capped C₁₈ stationary phase.

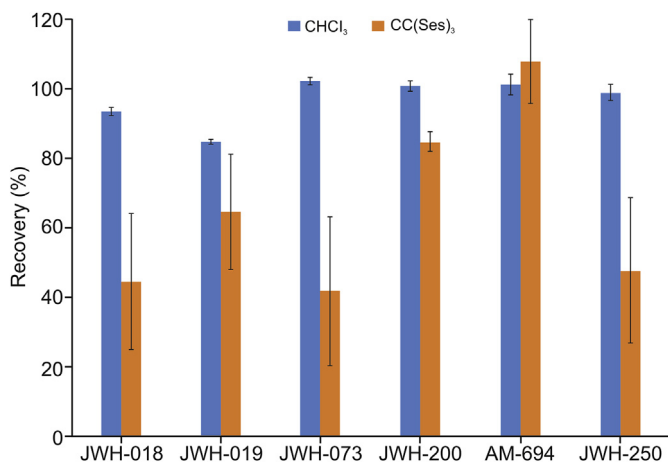


Fig. 3. Comparison between two DLLME procedures based on the use of chloroform and the deep eutectic solvent chlorine chloride(sesamol)₃ as extractants. In this case, the chlorinated solvent offers better recovery yields for most analytes. DLLME: dispersive liquid-liquid microextraction.

LODs and LLOQs were in the range of 2–21 pg/mL and 4–35 pg/mL, respectively, and were calculated via the analysis of five replicates, after preliminary experiments aimed at determining the spike levels detectable and quantifiable with a signal-to-noise ratio of 3 and 5, respectively.

For the recovery evaluation, in addition to the five replicates at the LLOQ and 10LLOQ spike levels, another aliquot was spiked post-extraction with the same nominal concentrations of analytes. All aliquots were processed and analyzed (Sections 2.2 and 2.5). For each analyte, the recovery was calculated by evaluating the ratio of the chromatographic areas: R_i (%) = (A pre-extraction/A post-extraction) × 100; then, the mean recovery was calculated as $(\bar{R} = \frac{\sum_{i=1}^5 R_i}{5})$.

The same experiments planned for the recovery were used to determine method precision: intra-day when performed within the same analytical session, and the inter-day when executed in two different analytical sessions (over two weeks). In all cases, the relative standard deviation (RSD) was less than 18%.

3.4. Comparison with other extraction methods

The main figures of merit (recovery, precision, LOD) of the validated method were compared with those of previous methods,

Table 2
Validation results ($n=5$).

Analytes	LOD (ng/mL)	LLOQ (ng/mL)	Recovery (%)		Intra-day precision (RSD, %)		Matrix-matched calibration curve	R^2
			LLOQ ^a	10LLOQ ^a	LLOQ ^a	10LLOQ ^a		
JWH-200	0.002	0.004	95	88	13	4	$y=39.207x-19.16$	0.9914
AM-694	0.008	0.013	81	97	18	10	$y=37.302x-28.351$	0.9948
JWH-250	0.006	0.009	73	87	14	8	$y=98.229x-10.088$	0.9977
JWH-073	0.021	0.035	93	101	16	12	$y=24.024x-2.9742$	0.9985
JWH-018	0.010	0.016	85	75	11	11	$y=55.062x-20.73$	0.9992
JWH-019	0.018	0.030	85	91	16	6	$y=32.24x-15.659$	0.9988

^a Spike levels values applied for the calculation of recovery and precision.

based on other extraction techniques and developed to isolate some SCs from oral fluid [17–21] (Table 3). Overall, our procedure is appealing owing to its good general performance. The LODs were up to 10 times lower [17–21], except for a few cases for which analogous values were determined. The recoveries were higher on average, but the SPE-based method showed better yields even if JWH-018 was recovered with an anomalously high value [20]. As far as precision is concerned, only two methods exhibit better figures [19,20]. Nevertheless, the present method has proved to be effective at low concentrations as recovery and precision were evaluated at significantly lower spike levels (from 100 to 1000 times lower than those of the other methods [17–21]). Regarding extraction time, our procedure is more rapid and simpler. The only exceptions are the “dilute and shoot” approach [19] and the one based on “deproteinization with ice acetonitrile” [21], which, however, provided a worse clean-up of the extracts.

Finally, we also performed an in-lab comparison using two different SPE-clean up procedures and the same HPLC-MS/MS instrumental method. The comparison was limited to the evaluation of recovery efficiency. The preliminary step to precipitate proteins was the same as that optimized for the DLLME procedure: 0.5 mL of a spiked oral fluid (at LLOQ) was treated with 1 mL of acetonitrile and, after centrifugation, the supernatant was removed and diluted with Milli-Q water up to 50 mL. Then, the diluted supernatant was loaded onto an Oasis HLB cartridge, and the analytes were eluted with 9 mL of methanol:dichloromethane (50:50, V/V). Evaporation and reconstitution were performed as described in the DLLME procedure. The results, evaluated using three replicates,

showed recoveries between 63% and 68%, except for JWH-019 (39%). Another sorbent which was tested was buckypaper, used as a membrane to perform stir-disc SPE [31–33]. In this case, the buckypaper disc was submerged into the diluted supernatant (50 mL) and left overnight under magnetic stirring, to favor analyte sorption; analyte desorption was performed using 9 mL of methanol:dichloromethane (50:50, V/V). Herein, the average recoveries were markedly high, ranging between 65.2% and 94.6% (three replicates). Surprisingly, JWH-200 was not recovered, probably due to its basic nature and the steric hindrance of the morpholine ring. In conclusion, the DLLME method is an advantageous alternative to perform routine analytical tasks in clinical and forensic toxicology laboratories, as demonstrated when compared with several different extraction techniques and procedures.

4. Conclusions

In the present study, an original DLLME procedure, resulting from a combination with a preliminary deproteinization step, was developed to isolate SCs from the oral fluid. The analysis of this matrix appears simple only at the surface, as the presence of peptides and proteins makes it substantially challenging. Their tendency to precipitate hinders the DLLME process, while their occurrence in the final extract can stress the HPLC-MS system, with a negative impact on both the column life and the instrumental signal. Hence, their exhaustive removal was performed in the developed procedure. To this end, acetonitrile was identified as a suitable solvent to perform the dual role of protein-denaturing and

Table 3
Comparison of some recent methods through their main figures of merit.

Method	Common analytes	Recovery (%) (spike level)	Intra-day precision (RSD, %) (spike level)	Time per sample (min)	LOD (ng/mL)	Refs.
LLE-LC-MS/MS (protein precipitation with ethanol followed by liquid-liquid extraction; evaporation)	JWH-200, AM-694, JWH-250, JWH-073, JWH-018, JWH-019	48.6–81.3 (0.3 ng/mL)	10.2–14.4 (0.3 ng/mL)	~ 120	0.015–0.030	[17]
SPE-LC-MS/MS (sample acidification; Strata-X, elution with 2-propanol:dichloromethane:acetic acid (24.5:75:0.5, V/V/V); evaporation)	JWH-200, JWH-250, JWH-073, JWH-018	56–99 (3 ng/mL)	1.8–25 (3 ng/mL)	~ 30	0.025	[18]
Dilute and shoot-LC-MS/MS (dilution with an extraction buffer and centrifugation)	JWH-200, JWH-018, JWH-073	68–70 (5 ng/mL)	< 10% (5 ng/mL)	~10	0.1	[19]
SPE-LC-MS/MS (sample acidification; elution with hexane/glacial acetic acid (98:2, V/V, 2 mL); evaporation)	JWH-018, JWH-073, JWH-250, JWH-200	96–122 (4 ng/mL) JWH-200 was not recovered and removed by the method	2.5–5.6 (4 ng/mL)	~ 30	0.5	[20]
Deproteinization-LC-MS/MS (protein precipitation using ice-cold acetonitrile; centrifugation; evaporation)	JWH-200, AM-694, JWH-250, JWH-073, JWH-018, JWH-019	72.5–77.7	4.1–11.2	~10	0.02–0.40	[2]
DLLME-LC-MS/MS (protein precipitation with acetonitrile, used as dispersing solvent for DLLME; extraction solvent: chloroform; evaporation)	JWH-200, AM-694, JWH-250, JWH-073, JWH-018, JWH-019	73–95 (0.004–0.035 ng/mL)	11–18 (0.004–0.035 ng/mL)	~15	0.002–0.021	This work

dispersing agents. High recovery efficiencies were obtained by selecting chloroform as the extraction solvent, which was more efficient than the LTTM chlorine chloride(sesamol)₃. On comparing SPE using Oasis HLB and buckypaper, the DLLME procedure was proved to be advantageous owing to its general performance and rapidity. Finally, this study highlights the superior selectivity of the bidentate C₁₈ silica hydride column and the particular chromatographic behavior of JWH-200, which distinguishes itself from other SCs as less hydrophobic and slightly basic. The isocratic separation on this column was set up to separate all analytes at the baseline within 14 min, providing a method that, as a whole, is advantageous for clinical and forensic routine analyses.

Declaration of competing interest

The authors declare that there are no conflicts of interest.

Acknowledgments

This work was supported by the Sapienza University of Rome through the project RICERCA 2019 (protocol number: RG11916B6451D44A).

Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.jpha.2020.11.004>.

References

- [1] D. Debruyne, R. Le Boisselier, Emerging drugs of abuse: current perspectives on synthetic cannabinoids, *Subst. Abuse Rehabil.* 6 (2015) 113–129.
- [2] J.W. Huffman, D. Dai, B.R. Martin, et al., Design, synthesis and pharmacology of cannabimimetic indoles, *Bioorg. Med. Chem. Lett.* 4 (1994) 563–566.
- [3] D. Favretto, J.P. Pascali, F. Tagliaro, New challenges and innovation in forensic toxicology: focus on the “New Psychoactive Substances”, *J. Chromatogr. A* 1287 (2013) 84–95.
- [4] K.A. Seely, J. Lapoint, J.H. Moran, et al., Spice drugs are more than harmless herbal blends: a review of the pharmacology and toxicology of synthetic cannabinoids, *Prog. Neuro-Psychopharmacol. Biol. Psychiatry* 39 (2012) 234–243.
- [5] N. Schaefer, M. Kettner, M.W. Laschke, et al., Simultaneous LC-MS/MS determination of JWH-210, RCS-4, Δ (9)-tetrahydrocannabinol, and their main metabolites in pig and human serum, whole blood, and urine for comparing pharmacokinetic data, *Anal. Bioanal. Chem.* 407 (2015) 3775–3786.
- [6] C. Marchioni, T.M. Vieira, A.E.M. Crotti, et al., In-tube solid-phase microextraction with a dummy molecularly imprinted monolithic capillary coupled to ultra-performance liquid chromatography-tandem mass spectrometry to determine cannabinoids in plasma samples, *Anal. Chim. Acta* 1099 (2019) 145–154.
- [7] I. Möller, A. Wintermeyer, K. Bender, et al., Screening for the synthetic cannabinoid JWH-018 and its major metabolites in human doping controls, *Drug Test. Anal.* 3 (2011) 609–620.
- [8] S. Odoardi, M. Fisichella, F.S. Romolo, et al., High-throughput screening for new psychoactive substances (NPS) in whole blood by DLLME extraction and UHPLC-MS/MS analysis, *J. Chromatogr. B* 1000 (2015) 57–68.
- [9] S. Dresen, N. Ferreirós, M. Pütz, et al., Monitoring of herbal mixtures potentially containing synthetic cannabinoids as psychoactive compounds, *J. Mass Spectrom.* 45 (2010) 1186–1194.
- [10] S. Hudson, J. Ramsey, L. King, et al., Use of high-resolution accurate mass spectrometry to detect reported and previously unreported cannabimimetics in “herbal high” products, *J. Anal. Toxicol.* 34 (2010) 252–260.
- [11] N. Uchiyama, R. Kikura-Hanajiri, J. Ogata, et al., Chemical analysis of synthetic cannabinoids as designer drugs in herbal products, *Forensic Sci. Int.* 198 (2010) 31–38.
- [12] G. Merola, Z. Aturki, G. D’Orazio, et al., Analysis of synthetic cannabinoids in herbal blends by means of nano-liquid chromatography, *J. Pharmaceut. Biomed. Anal.* 71 (2012) 45–53.
- [13] R. Kronstrand, L. Brinkhagen, C. Birath-Karlsson, et al., LC-QTOF-MS as a superior strategy to immunoassay for the comprehensive analysis of synthetic cannabinoids in urine, *Anal. Bioanal. Chem.* 406 (2014) 3599–3609.
- [14] K.B. Scheidweiler, M.A. Huestis, Simultaneous quantification of 20 synthetic cannabinoids and 21 metabolites, and semi-quantification of 12 alkyl hydroxy metabolites in human urine by liquid chromatography-tandem mass spectrometry, *J. Chromatogr. A* 1327 (2014) 105–117.
- [15] T.D. Freijo Jr., S.E. Harris, S.V. Kala, A rapid quantitative method for the analysis of synthetic cannabinoids by liquid chromatography-tandem mass spectrometry, *J. Anal. Toxicol.* 38 (2014) 466–478.
- [16] K.B. Scheidweiler, M.J. Jarvis, M.A. Huestis, Nontargeted SWATH acquisition for identifying 47 synthetic cannabinoid metabolites in human urine by liquid chromatography-high-resolution tandem mass spectrometry, *Anal. Bioanal. Chem.* 407 (2015) 883–897.
- [17] S. Kneisel, V. Auwärter, J. Kempf, Analysis of 30 synthetic cannabinoids in oral fluid using liquid chromatography-electrospray ionization tandem mass spectrometry, *Drug Test. Anal.* 5 (2013) 657–669.
- [18] A. de Castro, B. Piñeiro, E. Lendoiro, et al., Quantification of selected synthetic cannabinoids and Δ 9-tetrahydrocannabinol in oral fluid by liquid chromatography-tandem mass spectrometry, *J. Chromatogr. A* 1295 (2013) 99–106.
- [19] W.C. Rodrigues, P. Catbagan, S. Rana, et al., Detection of synthetic cannabinoids in oral fluid using ELISA and LC-MS-MS, *J. Anal. Toxicol.* 37 (2013) 526–533.
- [20] C. Coulter, M. Garnier, C. Moore, Synthetic cannabinoids in oral fluid, *J. Anal. Toxicol.* 35 (2011) 424–430.
- [21] S. Kneisel, M. Speck, B. Moosmann, et al., LC/ESI-MS/MS method for quantification of 28 synthetic cannabinoids in neat oral fluid and its application to preliminary studies on their detection windows, *Anal. Bioanal. Chem.* 405 (2013) 4691–4706.
- [22] M. Williams, J. Martin, P. Galetti, A validated method for the detection of synthetic cannabinoids in oral fluid, *J. Anal. Toxicol.* 43 (2019) 10–17.
- [23] E.G. Primel, S.S. Caldas, L.C. Marube, et al., An overview of advances in dispersive liquid-liquid microextraction for the extraction of pesticides and emerging contaminants from environmental samples, *Trends Environ. Anal. Chem.* 14 (2017) 1–18.
- [24] P. Tomai, A. Lippiello, P. D’Angelo, et al., A low transition temperature mixture for the dispersive liquid-liquid microextraction of pesticides from surface waters, *J. Chromatogr. A* 1605 (2019), 360329.
- [25] M.L. de Oliveira, B.A. Rocha, V.C. de Oliveira Souza, et al., Determination of 17 potential endocrine-disrupting chemicals in human saliva by dispersive liquid-liquid microextraction and liquid chromatography-tandem mass spectrometry, *Talanta* 196 (2019) 271–276.
- [26] F. Abujaber, A.I.C. Ricardo, Á. Rios, et al., Ionic liquid dispersive liquid-liquid microextraction combined with LC-UV-Vis for the fast and simultaneous determination of cortisone and cortisol in human saliva samples, *J. Pharmaceut. Biomed. Anal.* 165 (2019) 141–146.
- [27] P. Fernández, M. Regenjo, A. Ares, et al., Simultaneous determination of 20 drugs of abuse in oral fluid using ultrasound-assisted dispersive liquid-liquid microextraction, *Anal. Bioanal. Chem.* 411 (2019) 193–203.
- [28] J.J. Pesek, M.T. Matyska, R.I. Boysen, et al., Aqueous normal-phase chromatography using silica-hydride-based stationary phases, *Trac. Trends Anal. Chem.* 42 (2013) 64–73.
- [29] J.J. Pesek, M.T. Matyska, M.T. Hearn, et al., Temperature effects on solute retention for hydride-based stationary phases, *J. Separ. Sci.* 30 (2007) 1150–1157.
- [30] S.P. Humphrey, R.T. Williamson, A review of saliva: normal composition, flow, and function, *J. Prosthet. Dent.* 85 (2001) 162–169.
- [31] V. Pérez-Fernández, A. Gentili, A. Martinelli, et al., Evaluation of oxidized buckypaper as material for the solid phase extraction of cobalamins from milk: its efficacy as individual and support sorbent of a hydrophilic-lipophilic balance copolymer, *J. Chromatogr. A* 1428 (2016) 255–266.
- [32] P. Tomai, A. Martinelli, S. Morosetti, et al., Oxidized Buckypaper for stir-disc solid phase extraction: evaluation of several classes of environmental pollutants recovered from surface water samples, *Anal. Chem.* 90 (2018) 6827–6834.
- [33] P. Tomai, A. Martinelli, T. Gasperi, et al., Rotating-disc micro-solid phase extraction of F2-isoprostanes from maternal and cord plasma by using oxidized buckypaper as sorbent membrane, *J. Chromatogr. A* 1586 (2019) 30–39.